



Eine gute Druckqualität kann nur erreicht werden, wenn die Vorgaben und Hinweise aus dem Druckfahrgang SIG eingehalten werden. Bitte stellen Sie sicher, dass die Druckfahrgänge in ihrem Hause und bei Ihren Agenturen bekannt ist und die Basis für die Designgestaltung darstellt. Folgende, kommentierte Punkte stellen eine Abweichung vom Leitfaden dar bzw. bilden ein Risiko für ein stabiles, reproduzierbares Design. Sofern keine Änderung möglich ist, werden wir Ihnen wir Ihre Reklamationen aus daraus folgenden Qualitätsbeeinträchtigungen akzeptieren.



A good print quality can only be achieved if the requirements and instructions of the SIG artwork guideline are observed. Please make sure that the SIG artwork guideline is well-known for you and your agency. The SIG artwork guideline should be the basis for the design layout.

Abweichung vom Leitfaden stellt eine Abweichung von der guideline. They could be a risk for a stable and repeatable print results. If a required adaptation will be considered impossible or finally not desired by the customer, SIG CombiColor cannot be held responsible for printing problems and will consequently not accept any complaints accordingly.

- ☒ 8. Linienstärke und / oder Schriftart nicht gemäß SIG Leitfaden
Line width and / or font style not according to guideline

Rapport 188 mm
cb 4 1500ml

Possible longitudinal seam tolerance in bulk production

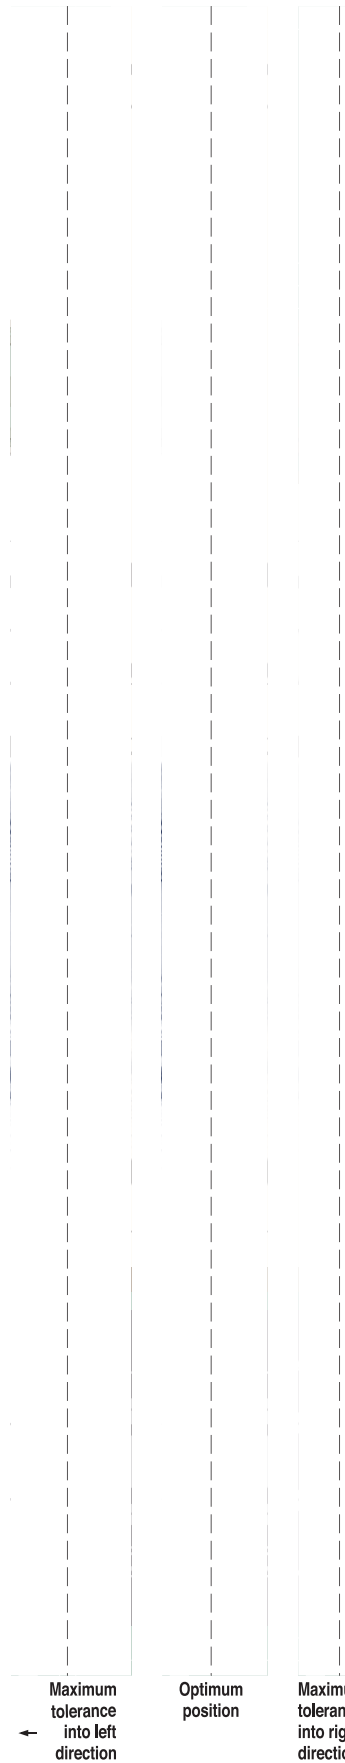

Janoschka Janoschka Deutschland GmbH Mattweg 1 77971 Kippenheim, Germany Tel.: (+49) 07825 / 849-0 Fax: (+49) 07825 / 2306		Customer: SIG Combibloc GmbH - Linnich / DE Job Title: Santa Helena Santa Helena Vino Blanco Keyline Nr.: cb4 1500ml / 596 783 Job Size: +395.8mm x +278.mm		Process: Tiefdruck Cust Ordnr.: 51773682 Repro-AV: Denis Arnolt (tel.) Operator: LH Data Nr.: 220		Janoschka Nr. S10023689-I Version 1 24.01.2024		Approval Although this design has been checked in compliance with our quality procedures, errors can occur. It is the customers responsibility to check this design for content, size, layout and colour separation before final approval to print.	
No color match on contract proof (see separate sample)									
1 C00096 INK COV: 14.8% 75% 50% 25% 5% 4% 3% 2% 1% S10023689-RP-1UP.ap		2 C00282 INK COV: 10.9% 75% 50% 25% 5% 4% 3% 2% 1% S10023689-RP-1UP.ap		3 C00235 INK COV: 5.8% 75% 50% 25% 5% 4% 3% 2% 1% S10023689-RP-1UP.ap		Output by: Ihoffmann Internal Approval Signature:			
4 C00231 INK COV: 1.7% 75% 50% 25% 5% 4% 3% 2% 1% S10023689-RP-1UP.ap		5 Black C00004 INK COV: 5.4% 75% 50% 25% 5% 4% 3% 2% 1% S10023689-RP-1UP.ap		leer INK COV: 0.1% 75% 50% 25% 5% 4% 3% 2% 1%		Customer Approval Signature:  25-01-24			